

Siemens Healthcare Diagnostics, a global leader in clinical diagnostics, provides healthcare professionals in hospital, reference, and physician office laboratories and point-of-care settings with the vital information required to accurately diagnose, treat, and monitor patients. Our innovative portfolio of performance-driven solutions and personalized customer care combine to streamline workflow, enhance operational efficiency, and support improved patient outcomes.

ADVIA Centaur, Dimension ExL, Dimension Vista, IMMULITE, and all associated marks are trademarks of Siemens Healthcare Diagnostics Inc. All other trademarks and brands are the property of their respective owners. Product availability may vary from country to country and is subject to varying regulatory requirements. Please contact your local representative for availability.

Order No. A91DX-CAI-121231-GC1-4A00
12-2012 | All rights reserved
© 2012 Siemens Healthcare Diagnostics Inc.

Global Siemens Headquarters

Siemens AG
Wittelsbacherplatz 2
80333 Muenchen
Germany

Global Siemens Healthcare

Headquarters
Siemens AG
Healthcare Sector
Henkestrasse 127
91052 Erlangen
Telephone: +49 9131 84-0
Germany
www.siemens.com/healthcare

Global Division

Siemens Healthcare Diagnostics Inc.
511 Benedict Avenue
Tarrytown, NY 10591-5005
USA
www.siemens.com/diagnostics

White Paper

Functional Sensitivity of Seven Automated Thyroid Stimulating Hormone Immunoassays

William E. Owen, ARUP Institute for Clinical and Experimental Pathology,[®] Salt Lake City, UT
Mary Lou Gantzer and Jeremy M. Lyons, Siemens Healthcare Diagnostics, Newark, DE
Alan L. Rockwood and William L. Roberts, Department of Pathology, University of Utah Health Sciences Center, Salt Lake City, UT

Abstract

Background

Serum thyroid stimulating hormone (TSH) measurements are useful for detecting clinical and subclinical primary hypo- and hyperthyroidism in ambulatory patients. For diagnosis of hyperthyroidism, the functional sensitivity (FS) is an important performance criterion, and current guidelines recommend an FS of ≤ 0.02 m IU/l for “third” generation performance.

Methods

We evaluated TSH FS for the Access 2, ADVIA Centaur®, Architect i2000, Dimension® ExL, Modular Analytics E170, IMMULITE® 2000 and Dimension Vista® 1500 automated immunoassays using serum pools tested over a 6-week period using 2 reagent lots and 2 calibrations. FS was determined by fitting a power function to the imprecision data using KaleidaGraph software.

Results

The FS (m IU/l) for Access 2, ADVIA Centaur, ARCHITECT i2000, Dimension ExL, Modular Analytics E170, IMMULITE 2000, and Dimension Vista 1500 systems were determined to be 0.039, 0.006, 0.007, 0.003, 0.008, 0.003, and 0.003, respectively. The lowest and next to lowest pools had overall mean TSH concentrations of 0.012 m IU/l and 0.020 m IU/l, respectively, and a range of concentrations of 0.005 to 0.022 m IU/l and 0.007 to 0.077 m IU/l, respectively.

Conclusions

All assays showed excellent performance in FS consistent with a “third” generation claim except for the Access 2 system. Further harmonization of TSH immunoassays is required, especially at lower concentrations.

Introduction

Most currently available automated thyroid stimulating hormone (TSH) immunoassays have a “third” generation claim, meaning a functional sensitivity (FS) of ≤ 0.02 m IU/l as recommended by the National Academy of Clinical Biochemistry.¹ These assays, because of their sensitivity and specificity, are acceptable for use in the diagnosis of thyroid disease from overt hypothyroidism to overt hyperthyroidism. In hospitalized patients, “third” generation assays help to distinguish sick hyperthyroid patients with very low values of TSH (0.05 m IU/l) from patients with mild temporal TSH reduction (0.05–0.1 m IU/l) consistent with non-thyroidal illness.² Clinical decisions may be guided or altered for patients with hyperthyroidism based on TSH results. Decisions about the dosing of exogenous thyroid hormone to patients with subnormal TSH can be aided by accurate quantification of TSH values 0.1 m IU/l.^{3,4} A study on the performance characteristics including FS of six TSH immunoassays having a “third” generation claim was published in 2005.⁵ Results of this study indicated the need for further efforts to harmonize TSH immunoassays including improved comparability at low TSH concentrations (0.2 m IU/l). Steps are being taken to achieve this goal.⁶ It was the purpose of our study to determine current FS performance of seven commercially available automated immunoassays and evaluate comparability at low TSH concentrations.

Materials and Methods

Seven automated TSH immunoassay analyzers were used in our study including Access 2 (Beckman Coulter), ADVIA Centaur (Siemens Healthcare Diagnostics), Architect i2000 (Abbott Diagnostics), Dimension ExL (Siemens), Modular Analytics E170 (Roche Diagnostics), IMMULITE 2000 and Vista 1500 (Siemens) systems. All immunoassays studied use chemiluminescent or electrochemiluminescent detection and are standardized to the World Health Organization Second International Reference Preparation (80/558).⁷ Testing on the Access 2, Architect i2000, Modular Analytics E170, and IMMULITE 2000 analyzers was performed at ARUP. The ADVIA Centaur, Dimension ExL, and Vista 1500 testing was performed at Siemens.

Our imprecision study met the requirements of the Clinical and Laboratory Standards Institute EP 17-A Protocol.⁸ Serum samples from individual subjects of 1–1.25 ml were obtained from a commercial supplier (vendor); a TSH value was supplied with each sample (tested primarily by a Modular Analytics E170 or an

ADVIA Centaur system). Seven pools with the required volume for the imprecision study were each prepared by combining 17–21 samples with comparable TSH concentrations. These seven prepared pools were aliquoted and all aliquots were stored frozen at -70 °C until time of testing. Imprecision was evaluated over 12 days of testing using 2 lots of reagent and 2 instrument calibrations. Seven aliquots per pool (one per immunoassay method) were thawed per day and assayed with one replicate per run, one run per day, 2 days per week, and 3 weeks per reagent lot for a total of 12 replicates.

In order to determine the FS, a power function was fitted to the imprecision data using four different software packages: KaleidaGraph (Kaleida), Graph Pad Prism (Prism), CricketGraph (Cricket), and Microsoft Excel 2007 (Excel). PSI-Plot software was used to simulate different data analysis routines to determine the source of differences in calculated FS between Kaleida, Prism, Cricket, and Excel.

Table 1. Summary of functional sensitivity (FS) analyses.

Software	Kaleida	Prism	Cricket	Excel	PSI-Plot (Natural Space) ^a	PSI-Plot (Quasi Natural Space) ^b	PSI-Plot (In In Space) ^c
Functional Sensitivity	m IU/l (r)	m IU/l (r)	m IU/l (r)	m IU/l (r)	m IU/l (r)	m IU/l (r)	m IU/l (r)
Instrument							
Access 2	0.031 ^d , 0.039 ^e (0.850) ^d , (0.655) ^e	0.037 ^d , 0.049 ^e (0.869) ^d , (0.656) ^e	0.039 (0.690)	0.039 (0.688)	0.037 ^d , 0.049 ^e (0.877) ^d , (0.658) ^e	0.039 (0.657)	0.039 (0.690)
ADVIA Centaur	0.006 (0.835)	0.009 (0.842)	0.006 (0.894)	0.006 (0.894)	0.010 (0.844)	0.006 (0.835)	0.006 (0.894)
ARCHITECT i2000	0.007 (0.914)	0.006 (0.914)	0.007 (0.958)	0.007 (0.958)	0.006 (0.913)	0.007 (0.913)	0.007 (0.958)
Dimension ExL	0.003 (0.954)	0.006 (0.971)	0.004 (0.946)	0.004 (0.946)	0.006 (0.976)	0.004 (0.954)	0.004 (0.946)
Modular Analytics E170	0.008 (0.982)	0.008 (0.944)	0.008 (0.978)	0.007 (0.978)	0.009 (0.983)	0.008 (0.981)	0.008 (0.978)
IMMULITE 2000	0.003 (0.744)	0.008 (0.748)	0.003 (0.782)	0.003 (0.781)	0.006 (0.750)	0.003 (0.742)	0.003 (0.782)
Dimension Vista 1500	0.003 (0.862)	0.008 (0.940)	0.003 (0.840)	0.003 (0.841)	0.008 (0.963)	0.003 (0.862)	0.003 (0.840)

a. PSI-Plot fit in “natural space” was performed using a user-defined true nonlinear fit with original data.
 b. PSI-Plot fit in “quasi natural space” was performed using a pre-defined, built in power law data fitting capability.
 c. PSI-Plot fit in “In In space” was performed after both variables were transformed by a natural log function.
 d. Fit excluding Pool 2 result.
 e. Fit using all 7 pool results.

Results

The results for FS calculations by Kaleida, Prism, Cricket, and Excel for the seven immunoassays are summarized in Table 1. This table also includes results for FS calculations by PSI-Plot determined using three different methods of analyzing the data. The fit for “natural space” was done using a user defined nonlinear equation (power law) to do a fit in natural variable space with the original data. The calculation using “quasi natural space” was carried out by using a pre-defined built in power law ($y = a \cdot x^b$) fitting capability in the PSI-Plot software using the original data. The “In In space” (i.e. natural log) fit was performed as follows: both axes were transformed by taking the natural log of the data, then the data were fit by ordinary linear regression, and finally the parameters from the fit were transformed back to ordinary variable space. Fig. 1 shows a comparison of power curve fitting by Kaleida and Prism of results for the Access 2 system. In panels A and C all seven pool results are shown. In panels B and D results for Pool 2 were excluded. Pool 2 (see arrow in panels A and C) could not be excluded as a statistical outlier but was considered a visual outlier. The data for the Access 2 system in Table 1 using Kaleida and Prism are summarized from the results of the power curve calculations (see statistics in Figure 1 caption).

The lowest pool (Pool 1) had mean TSH concentrations of 0.022, 0.016, 0.008, 0.005, 0.007, 0.015, and 0.008 m IU/l for Access 2, ADVIA Centaur, Architect i2000, Dimension ExL, Modular Analytics E170, IMMULITE 2000, and Vista 1500 systems, respectively. The next to lowest pool (Pool 2) had mean TSH concentrations for Access 2, ADVIA Centaur, Architect i2000, Dimension ExL, Modular Analytics E170, IMMULITE 2000, and Vista 1500 of 0.077, 0.014, 0.010, 0.007, 0.009, 0.016, and 0.010 m IU/l, respectively. The comparison of mean TSH concentrations for each pool by each method is shown (Figure 2). The arrow in Figure 2 indicates the Access 2 value for Pool 2 that was considered a divergent visual outlier as discussed above.

Discussion


All immunoassays we studied had an FS consistent with a “third” generation claim (0.02 m IU/l) except for the Access 2 system. Results summarized in Table 1 indicated that Access 2 had FS 0.02 m IU/l whether Pool 2 was included or excluded, and whether or not the claim was met did not depend on the software used for analysis.

There are at least four variables that contribute to FS variability. These include the performance of the analyzer that is used if it has not been properly maintained, the reagent lots that are used, the characteristics of the patient pools that are tested, and software that is used to construct the power curve. In the current study, all instruments used were maintained according to manufacturer recommendations and the same sample pools and power curve software were also used across all instruments.

The results for Access 2 contrast with an earlier study where an FS of 0.020 m IU/l was obtained, while the Architect i2000, Modular Analytics E170, and IMMULITE 2000 gave comparable results.⁵ This study used Cricket for power curve analysis and determination of FS. The Access 2 method gave an FS of 0.028 m IU/l in a study conducted in 1997.⁹ The reason for differences in Access 2 performance in each of the three studies is unclear.

The ADVIA Centaur FS result of 0.006 m IU/l contrasted with an earlier study where the FS was 0.039 m IU/l.⁵ The Centaur TSH assay in the previous study has since been reformulated to improve the FS; the reformulated assay was used in the current study, and as expected, a lower FS was obtained.

Figure 1. Comparison of Prism versus Kaleida analyses of Access 2 Results.

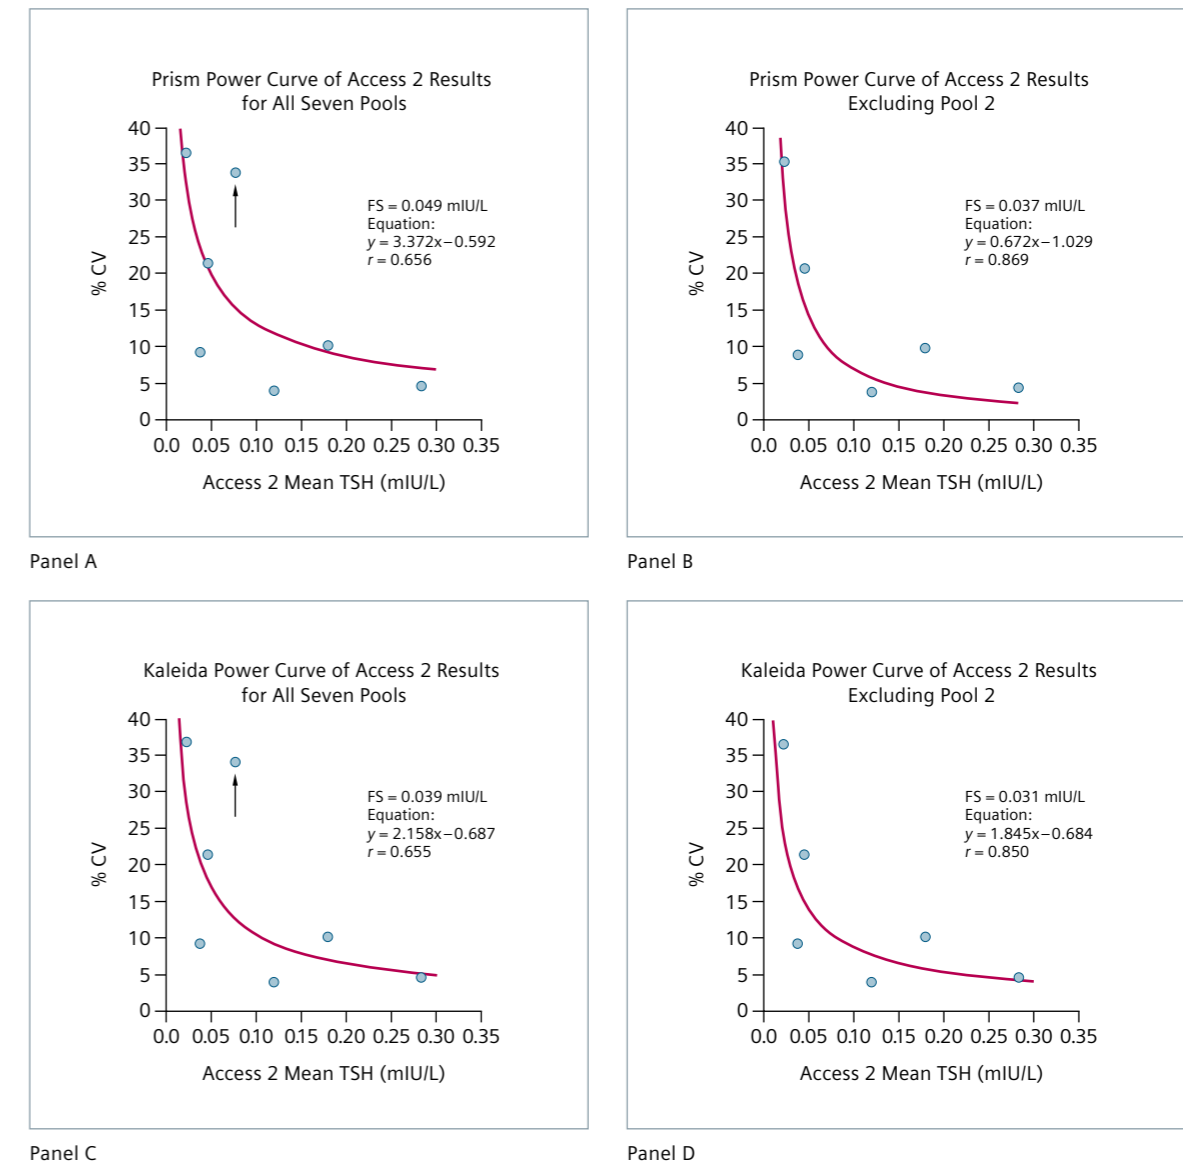


*Corresponding author at:
 c/o ARUP Laboratories, 500 Chipeta Way, Salt Lake City, UT 84108, USA.
 Telephone: +1-801-583-2787, x2086; fax: +1-801-584-5207.
 E-mail address: william.roberts@aruplab.com (W.L. Roberts).

Figure 2 indicates that the Access 2 assay had the highest recoveries of TSH, especially for samples with results 0.040 m IU/l. This was similar to previous study results.⁵ The Dimension ExL assay had the lowest TSH recoveries for samples with results 0.040 m IU/l. All methods gave more comparable results above 0.040 m IU/l (Figure 2). The health status of the patients whose samples were used to make our pools was not available. Those with low TSH were most likely from unhealthy individuals. The lack of comparability of the immunoassays seen at low TSH concentrations may in part be due to differences in antibody specificity, particularly for abnormal TSH isoforms.^{10,11} Our data indicate that harmonization of TSH immunoassays remains a challenge, though progress has been made.^{6,12}

Differences seen in calculated FS based on the software used (Table 1) were an interesting and unexpected result from our study. Based on results for both "ln ln space" and "quasi natural space" fit using the PSI-Plot software, we surmised that the "quasi-natural space" calculation followed the same log transform procedure as the "ln ln space" calculation we performed only it is done internally (hidden from the user). The results for "ln ln space" fit and "quasi natural space" fit are very similar to those calculated by Kaleida, Cricket, and Excel indicating that these software packages follow an internal procedure as seen with the "quasi natural space." The Prism software results paralleled those of the "natural space" calculations where the original data with no log transformation were used for curve fit. In comparing the power curves plotted by Prism and Kaleida for the Access 2 study results (Figure 1), we observed that the Pool 2 result affected the Prism curve (Figure 1, panels A and B) substantially more than the Kaleida curve (Figure 1, panels C and D).

Figure 2. Mean TSH concentrations for each pool and method. The mean concentration of each pool for each immunoassay plotted against pool number.

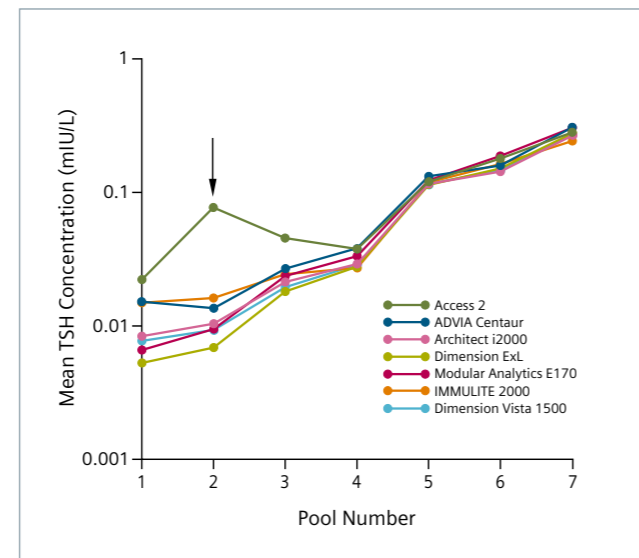

We speculated that the log transformation of the data makes the final calculated curve parameters more resistant to effects of divergent points. There were still uncertainties in how the different software packages performed the calculation for "r". However, it appeared that the calculation of "r" was done in the "natural space" for both Prism and the user programmed fit in PSI-Plot.

Our study indicated that the ADVIA Centaur, Architect i2000, Dimension ExL, Modular Analytics E170, IMMULITE 2000, and Vista 1500 TSH immunoassays have excellent performance with an FS consistent with a "third" generation claim. Further harmonization of TSH immunoassays is required, especially at lower TSH concentrations.

Acknowledgements

Siemens Healthcare Diagnostics provided reagents and support for this study. The Access 2, ARCHITECT i2000, and Modular Analytics E170 analyzers at ARUP were provided by Beckman Coulter, Abbott Diagnostics, and Roche Diagnostics, respectively. The ARUP Institute for Clinical and Experimental Pathology[®] provided support for this study.

References

- Baloch Z, Carayon P, Conte-Devolx B, et al. Laboratory medicine practice guidelines. Laboratory support for the diagnosis and monitoring of thyroid disease. *Thyroid*. 2003;13:3–126.
- Demers LM. Thyroid disease: pathophysiology and diagnosis. *Clin Lab Med*. 2004;24:19–28.
- Beckett G, MacKenzie F. Thyroid guidelines—are thyroid-stimulating hormone assays fit for purpose? *Ann Clin Biochem*. 2007;44:203–8.
- Witherspoon LR. Clinical utility of sensitive TSH measurements. *LabMedicine*. 2005;36:711–5.
- Rawlins ML, Roberts WL. Performance characteristics of six third-generation assays for thyroid-stimulating hormone. *Clin Chem*. 2004;50:2338–44.
- Thienpont LM, Van Uytvanghe K, Beastall G, et al. Report of the IFCC Working Group for standardization of thyroid function tests; part 1: thyroid-stimulating hormone. *Clin Chem*. 2010;56:902–11.
- Gaines Das RE, Bristow AF. The second international reference preparation of thyroid-stimulating hormone, human, for immunoassay: calibration by bioassay and immunoassay in an international collaborative study. *J Endocrinol*. 1985;104:367–79.
- Tholen DW, Linnet K, Kondratovich M, Armbruster DA, Garrett PE, Jones RL. Protocols for determination of limits of detection and limits of quantitation; approved guideline. NCCLS Document EP17-A CLSI, Pennsylvania, USA; 2004.
- d'Herbomez M, Sapin R, Gasser F, Schlienger JL, Wemeau JL. Two centre evaluation of seven thyrotropin kits using luminescent detection. *Eur J Clin Chem Clin Biochem*. 1997;35:609–15.
- Trojan J, Theodoropoulou M, Usadel KH, Stalla GK, Schaaf L. Modulation of human thyrotropin oligosaccharide structures—enhanced proportion of sialylated and terminally galactosylated serum thyrotropin isoforms in subclinical and overt primary hypothyroidism. *J Endocrinol* 1998;158:359–65.
- Thyrotropin/thyroid stimulating hormone (tsh) measurement. *Thyroid*. 2003;13:33–44.
- Donadio S, Pascual A, Thijssen JH, Ronin C. Feasibility study of new calibrators for thyroid-stimulating hormone (TSH) immunoprocures based on remodeling of recombinant TSH to mimic glycoforms circulating in patients with thyroid disorders. *Clin Chem*. 2006;52:286–97.

Reprinted From:

Owen, WE, et al, Functional sensitivity of seven automated thyroid stimulating hormone immunoassays, *Clin Chim Acta* (2011), doi: 10.1016/j.cca.2011.08.002. Adapted with Permission from Elsevier.